HORSELEY DENTAL

Tel: 02-8717 6500 Toll Free: 1300-130-718

E-mail: orders@horseley.com.au Website: www.horselev.com.au

Equipment

February 2023 FREE for orders over \$300.00

ALL PRICES GST INCLUSIVE prices and offers subject to change without notice
OFFERS ARE NOT VALID IN CONJUNCTION WITH ANY OTHER SPECIAL/BONUS OFFERS AND SUBJECT TO STOCK AVAILABILITY Goods sold are not returnable without prior approval. Returns and claims must be made within 10 days of delivery. Costs incurred by return goods will be

at the sender's expense. Goods returned for credit or exchange must be unmarked and in a saleable condition

All accounts are strictly 30 days from invoice date. We reserve the right to charge 2% interest per month on overdue accounts.

LOW SPEED HANDPIECES AND AIR MOTOR



L10-1 Straight Handpiece 1.1 Standard \$115.50



120-11 Latch CA Handpiece 1:1 Standard \$99.55



L20-1P **Push Button** CA Handpiece 1:1 Standard \$148.50



L20-1PM Push Button Mini Head CA Handpiece 1:1 Standard \$165.00



I 20-4P Push Button CA Handpiece 4:1 Reduction \$198.00

precisionplus



L20-4PM Push Button Mini Head CA Handpiece 4:1 Reduction



Air Motor (4 holes) 20,000 r.p.m.

Spare Heads L20L-A Latch

Buv 2

aet **FREE**

I 20P-A Push Button \$68.75 L20PM-A Push Button Mini \$79.75

12 MONTH WARRANTY

PROPHY LOW SPEED HANDPIECES



L20-1PY (SS) Screw-In / Snap-On CA Handpiece 1:1 Standard \$165.00



L20-4PY (SS) Screw-In / Snap-On CA Handpiece 4:1 Reduction



L20-4PY (R) 60° Turn Reciprocating Push Button Standard Head CA Handpiece 4:1 Reduction \$198.00

L20-4PY (RM) 60° Turn Reciprocating Push Button Mini Head CA Handpiece 4:1 Reduction \$198.00



Prophy Angle Straight Handpiece 4:1 Reduction

Spare Heads

L20PY (RM)-A Reciprocating Mini ... \$79.75

precisionplus



- Anti-retraction
- Ceramic Bearings
- · Stainless steel head
- Ergonomic design
- · Quiet operation noise level, less than 65 dB
- Autoclavable up to 134°C
- Midwest 4 holes

TURBINE STANDARD CONNECTION

T90P High Torque Push Button (Midwest 4 Holes) ... \$198.00 T90P(A) High Torque PB Cartridge\$99.55

12 MONTH WARRANTY





NON LED HIGH TORQUE TURBINE QUICK DISCONNECT
T90+QK Kavo¹ Type (without Coupling)\$599.50
T90+(A) High Torque PB Cartridge\$299.75

NON LED QUICK COUPLING QK Kavo¹ Type (non LED) w Spray Adjustment ... \$198.00 NON LED QUICK COUPLING

with Spray Adjustment



- Anti-retraction
- Ceramic Bearings
- · Stainless steel head
- Quiet operation noise level, less than 65 dB
- Ergonomic design
- Autoclavable up to 134°C
- Kavo¹ type fitting





- LED Fibre Optic
- Anti-retraction
- Ceramic Bearings
- Stainless steel head
- Quiet operation noise level, less than 65 dB
- Ergonomic design
- Autoclavable up to 134°C

precisionplus

Kavo¹ type fitting

1. KAVO is a registered trademark of Kavo Dental GmbH Germany

LED LIGHT BULBS

Life 200 times longer than halogen bulb, brighter light, Simple, Sterilizable, Less self-heating, Less wattage, Durable, Superior light quality ... Natural Daylight quality will let you NEVER want to go back to Halogen again!



KaVo MULTIflex LUX® Type \$38.50 W&H LED Type \$99.50



- Semiconductor LED
- Optimal 25,000 Lux illumination
- Daylight neutral 5,900-6,000 K colour temperature
- Voltage range 3.0 3.6 V DC
- Lifespan (Lifetime) > 10,000 hours
- Power Consumption < 50 mA

Lamp socket fitting tailored to handpieces or couplings. Please observe correct orientation to ensure correct electrical polarity.

If the LED shines red or not at all, remove and rotate the LED through 180 degrees, then replace

BEING AIR MOTOR AND LOW SPEED HANDPIECES 'E' FITTING INTERNAL SPRAY



12 MONTH WARRANTY



BEING LOW SPEED HANDPIECE AND HEADS INTERNAL SPRAY



MODERN FULL TITANIUM TURBINES STANDARD CERAMIC BEARINGS








EyeSpecial C-IV



Smart Dental Camera *Designed for the Entire Team*

FAST Precise Versatile

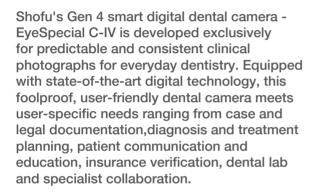

EyeSpecial Features...

9 pre-set dental shooting modes. Compact, ultra-light & easy to hold with one hand. Fast auto-focus with built-in anti-shake with image stabilization and anti-reflection features. Cutting edge Flashmatic System for True-colour reproduction with blockout of ambient light. Water, chemical and scratch resistant to prevent cross contamination. Brilliant display with fast & intuitive menu navigation. Video function, Micro HDMI connector, QR code features, and Trigger Flash Mode for portrait photography. Optional attachable cross polarizer.



E0021 EyeSpecial C-IV \$6,875.00/unit

SPECIAL \$5,995.00 per unit


Easy, Intuitive Navigation

Operating EyeSpecial C-IV is virtually effort less and eliminates the need for prior photography knowledge or extensive training. The high-resolution 3.5" LCD touch screen panel with an intuitive menu and simple, uncomplicated icons guides users to easily select the appropriate option and capture consistent, quality clinical photos. Images can be instantly viewed on the display, assessed, edited with draw-edit function, communicated and archived conveniently.

Compact and Convenient

This ultralight, high-performance camera is ready to use, right out-of-the-box without requiring any "heavyweight"

accessories such as external flashes or interchangeable lenses. Easily operated with just one hand, it frees up the other to hold the cheek retractor or mirror during the dental photography.



Close up lens (49 mm) from Kenko 16 GB SDHC memory card SH0FU gray card Quick reference and instructions

Hand strap User's manual 4 AA batteries

E0022 Cross Polarizer \$995.50



CO1-M/CO2-M LED CURING LIGHTS MINI (with USB charger)

- 360° Rotatable tips
- Automatic compensation circuit for constant power output
- Fully covered membrane panel for easy cleaning and infection control
- Light weight:
- approx. 85 gms
 Dual modes: FULL / SOFT
- 12 Operation times
- Fully charged battery provides over 100 x 10 second curing cycles

CO1-M / CO2-M SPECIFICATIONS							
Model C01-M (F.O. Light Guide) C02-M (Direct Light Sou							
LIGHT TIP		8 mm (dia.)	11 mm (dia.)				
LIGHT WAVELENGTH		440~480 nm	440~480 nm				
FULL SOFT		1,200 mW/cm² for 5, 10, 15, 20, 25, 30 seconds±10%					
		1 st five seconds from 0-900 mW/cm ² next	t 5, 10, 15, 20, 25 seconds 900 mW/cm²±10%				
WEIGHT		86 gms	84 gms				
LENGTH		230 mm	220 mm				

C01-M / C02-M CURING LIGHT DEPTH OF CURE								
MODEL MODEL	(F.U. Light Guide) Manager Weasurements (Direct Light Source) Manager Weasurements							
FULL 10 seconds		4.3 mm	2.15 mm	10 seconds	5.1 mm	2.55 mm		
SOFT	15 seconds	4.6 mm	2.30 mm	15 seconds	4.8 mm	2.40 mm		

REMARKS: Above data is based on test results using an A2 shade composite. The light tip was placed above and pointed perpendicular to the composite. Tests were done as per ISO 4049 Standard. The samples were measured and the data was divided by two (50% of the total composite depth cured). ISO 4049 Standard requires that the results for class II restorative materials should be at least 1.5 mm for non-opaque shades and 1.0 mm for opaque shades. All resins and composites have different curing times. It is recommended that you should test your resins and composites performance to determine the curing times required.




AUTOCLAVABLE FIBRE OPTIC LIGHT GUIDE CAN RE **ROTATED 360°** ON/OFF **SWITCH** AUTOMATIC DISPLAY COMPENSATION **SCREEN** CIRCUIT FOR CONSTANT POWER OUTPUT TIME **SWITCH** MODE INDICATORS ●-SOFT CUSE MODE (M) SWITCH **FULLY COVERED** C01 MEMBRANE PANEL FOR EASY CLEANING AND INFECTION CONTROL A FULL CHARGE **OF BATTERY CAN BE USED MORE THAN** 100 TIMES WHEN SIZE: L265 x Dia.27 (mm) **SET AT 10 SECOND** TIME MODE REPLACEABLE **BATTERY** OPENING

CO1 LED CURING LIGHTS with fibre optic light guides

		C01 SPE	CIFICATIONS			
	Model	CO1-C (classic)	C01-S (super power)	C01-D (dual range)		
F.O.	LIGHT GUIDE	8 mm (dia.)	11 mn	ı (dia.)		
LIGH	T WAVELENGTH	440~480 nm	440~480 nm	440~480 nm		
A	PPLICATION	General	Ortho / General	General / Ortho		
	TACK	N/A	900 mW/cm² for 1 second±10%			
	TURBO	1,500 mW/cm² for 5 seconds ±10%	2,000 mW/cm² for 4 seconds±10%			
	3' + 3'	N/A	2,000 mW/cm² for 3 + 3 seconds±10% (with 1 second blink in between)			
MODE	6' + 6'	N/A	1,500 mW/cm² for 6 + 6 seconds±10% (with 1 second blink in between)			
_	FULL	1,200) mW/cm² for 5, 10, 15, 20 seconds±10%			
	RAMP	1 st five seconds from 0-1,20	00 mW/cm ² next 5, 10, 15, 20 seconds 1,200 mW/cm ² ±10%			
SOFT CURE		1 st five seconds from 0-900 n	N/cm ² next 5, 10, 15, 20, 25 seconds 900 mW/cm ² ±10%			
WEIGHT		205 gms	200 gms	200 gms		
LENGTH		260 mm	265 mm	265 mm		

	CURING LIGHT MODE APPLICATIONS						
TACK	A very short initial cure for temporary processing before the final cure. For example when removing excess materials whilst bonding veneers or using temporary cement. Tack rings are included inside the box.						
TURB0	Super fast curing for resin and composite that is no more than 2 mm thick. Also recommended for ceramic brackets, bonding veneers etc.						
3' + 3'	3 Second Mesial + 3 Second Distal for metal brackets resin bonding (with 1 second blink in-between)						
6' + 6'	6 Second Mesial + 6 Second Distal for metal brackets with bonding resin requiring more curing time and for buccal tube bonding (with 1 second blink in-between)						
FULL	For general applications						
RAMP	First 0–5 seconds are ramped for general application.						
SOFT CURE	First 0–5 seconds are ramped for more gentle processing, designed for patients sensitive to heat.						



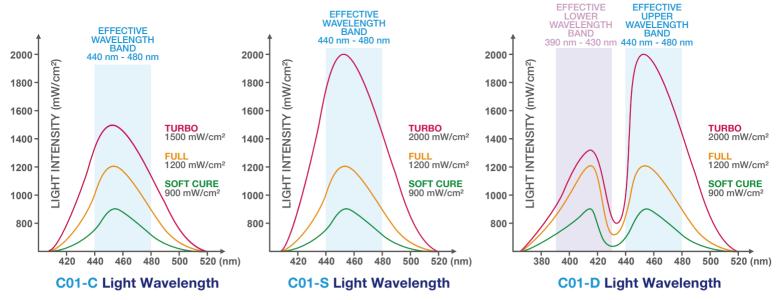

	C01-C / C01-S / C01-D CURING LIGHT DEPTH OF CURE								
MODEL	CO1-C (classic) Curing Time	Depth Measurements	ISO 4049 Depth Measurements (-50%)	C01-S (super power) Curing Time	Depth Measurements	ISO 4049 Depth Measurements (-50%)	C01-D (dual range) Curing Time	Depth Measurements	ISO 4049 Depth Measurements (-50%)
TURB0	5 seconds	4.2 mm	2.10 mm	4 seconds	4.6 mm	2.30 mm	4 seconds	4.3 mm	2.15 mm
FULL	10 seconds	4.3 mm	2.15 mm	10 seconds	5.1 mm	2.55 mm	10 seconds	4.4 mm	2.20 mm
RAMP	10 seconds	4.1 mm	2.05 mm	10 seconds	5.0 mm	2.50 mm	10 seconds	4.2 mm	2.10 mm
SOFT CURE	15 seconds	4.6 mm	2.30 mm	15 seconds	4.8 mm	2.40 mm	15 seconds	4.6 mm	2.30 mm


REMARKS: Above data is based on test results using an A2 shade composite. The light guide tip was placed above and pointed perpendicular to the composite. Tests were done as per ISO 4049 Standard. The samples were measured and the data was divided by two (50% of the total composite depth cured). ISO 4049 Standard requires that the results for class II restorative materials should be at least 1.5 mm for non-opaque shades and 1.0 mm for opaque shades. All resins and composites have different curing times. It is strongly recommended that you should test your composite and resin performance to determine the curing times required.

Data is only for reference, always follow the instructions from your resin and composite manufacturers.


- There are many variables (distance and angle between the light tip and composite, area, shade, thickness and type etc.) affecting
 composite curing times. It is recommended to place and cure a maximum of 2 mm for each composite placement.
- Using a barrier sleeve on the curing light will reduce 5-10% of light intensity.
- The light guide tip should be placed approximately 1-2 mm above the composite or resin and pointed perpendicular to the tooth surface.
- High intensity curing lights produce more heat. This is a direct indication of the power of the light being emitted. When using the
 device for more than 10 seconds, do not keep the light tip in one position. It is always recommended to use a dental syringe to blow
 a cold air flow on the area during long periods of curing. This will maintain a lower temperature for the composite and surrounding
 area, particularly when using rubber dam so as to avoid any rubber dam breakage due to heat built-up.
- Do not expose soft tissue to the light being emitted for more than 2 seconds or burns may occur.
- Avoid the light guide tip coming into contact with any soft tissue in the mouth.





CO2 LED CURING LIGHTS 90° right angle direct light source head

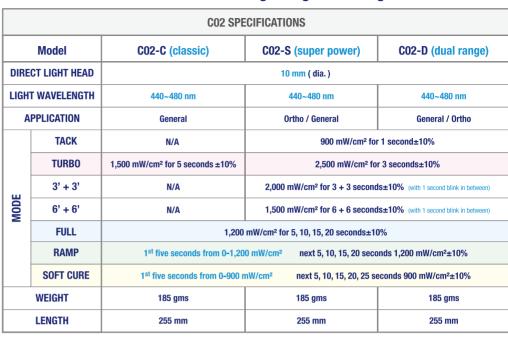

	CURING LIGHT MODE APPLICATIONS						
TACK A very short initial cure for temporary processing before the final cure. For example when removing excess materials whilst bonding veneers or using temporary cement. Tack rings are included inside							
TURB0	Super fast curing for resin and composite that is no more than 2 mm thick. Also recommended for ceramic brackets, bonding veneers etc.						
3' + 3' 3 Second Mesial + 3 Second Distal for metal brackets resin bonding (with 1 second blink in-between)							
6' + 6' 6 Second Mesial + 6 Second Distal for metal brackets with bonding resin requiring more curing time and for buccal tube bonding (with 1 second blink in-between)							
FULL	For general applications						
RAMP	First 0–5 seconds are ramped for general application.						
SOFT CURE	First 0–5 seconds are ramped for more gentle processing, designed for patients sensitive to heat.						

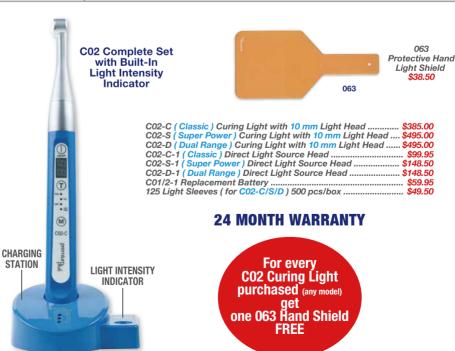

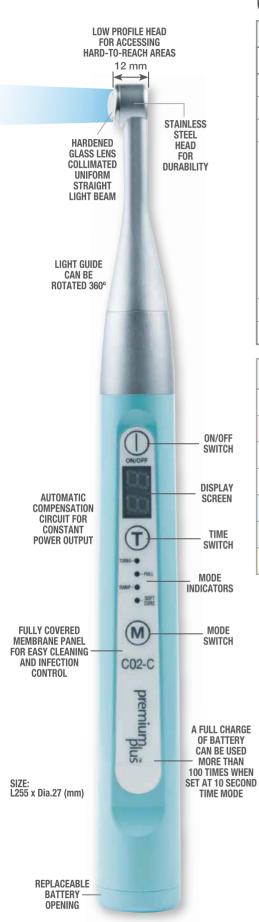

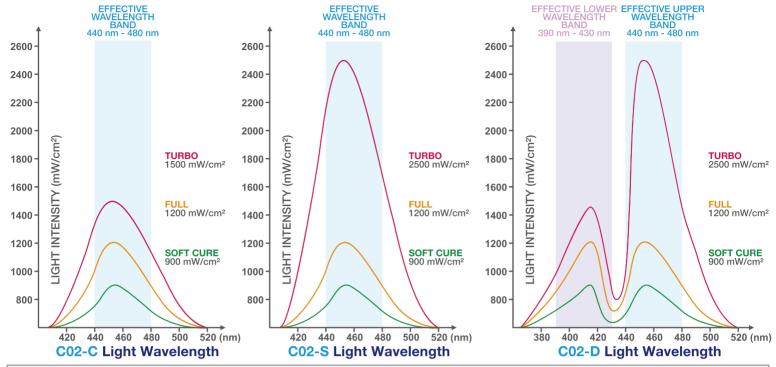

	CO2-C / CO2-S / CO2-D CURING LIGHT DEPTH OF CURE								
MODEL	CO2-C (classic) Curing Time	Depth Measurements	ISO 4049 Depth Measurements (-50%)	CO2-S (super power) Curing Time	Depth Measurements	ISO 4049 Depth Measurements (-50%)	CO2-D (dual range) Curing Time	Depth Measurements	ISO 4049 Depth Measurements (-50%)
TURB0	5 seconds	4.4 mm	2.20 mm	3 seconds	4.6 mm	2.30 mm	3 seconds	4.5 mm	2.25 mm
FULL	10 seconds	5.1 mm	2.55 mm	10 seconds	5.3 mm	2.65 mm	10 seconds	5.2 mm	2.60 mm
RAMP	10 seconds	4.8 mm	2.40 mm	10 seconds	5.3 mm	2.65 mm	10 seconds	4.9 mm	2.45 mm
SOFT CURE	15 seconds	5.0 mm	2.50 mm	15 seconds	5.4 mm	2.70 mm	15 seconds	5.1 mm	2.55 mm

REMARKS: Above data is based on test results using an A2 shade composite. The light tip was placed above and pointed perpendicular to the composite. Tests were done as per ISO 4049 Standard. The samples were measured and the data was divided by two (50% of the total composite depth cured). ISO 4049 Standard requires that the results for class II restorative materials should be at least 1.5 mm for non-opaque shades and 1.0 mm for opaque shades.

All resins and composites have different curing times. It is strongly recommended that you should test your composite and resin performance to determine the curing times required.

Data is only for reference, always follow the instructions from your resin and composite manufacturers.

- There are many variables (distance and angle between the light tip and composite, area, shade, thickness and type etc.) affecting composite curing times. It is recommended to place and cure a maximum of 2 mm for each composite placement.
 Using a barrier sleeve on the curing light will reduce 5-10% of light intensity.
 The light tip should be placed approximately 1-2 mm above the composite or resin and pointed perpendicular to the tooth surface.
 High intensity curing lights produce more heat. This is a direct indication of the power of the light being emitted. When using the device for more than 10 seconds, do not keep the light tip in one position. It is always recommended to use a dental syringe to blow a cold air flow on the area during long periods of curing. This will maintain a lower temperature for the composite and surrounding area, particularly when using rubber dam so as to avoid any rubber dam breakage due to heat built-up.
 Do not expose soft tissue to the light being emitted for more than 2 seconds or burns may occur.
 Avoid the light tip coming into contact with any soft tissue in the mouth. As an option, you may cover the entire curing light with a disposable sleeve and then place the Heat Protective Ring (included inside the packing box) onto the light tip covered with sleeve
- disposable sleeve and then place the Heat Protective Ring (included inside the packing box) onto the light tip covered with sleeve as shown below. Ensure the Heat Protective Ring is securely positioned on the curing light before starting the cure.





MaxPiezo 7+ (EMS Type) Portable LED Scaler Set\$880.00
MaxPiezo DS7+ (SATELEC Type) Portable LED Scaler Set ...\$880.00

REFINE MaxPiezo 7+ / DS7+ PORTABLE LED

- · Automatic frequency tracking, real-time feedback
- Extra large, capacity 600 ml water tank for water, chlorhexidine, hydrogen peroxide, sodium hypochlorite etc...
- Power and water controlled by touch panel, easy to clean for infection control
- Detachable handpiece
- Frequency: 28 kHz ± 3 kHz
- · Complete with 8 tips
- Size: W180mm x D180mm x H150mm
- Weight: 1.6 kg (unit only)
- · Colour: White



REFINE MaxPiezo 6+ / DS6+ LED SCALERS



- Power and water controlled by touch panel, easy to clean for infection control
- Detachable handpiece
- Frequency: 28 kHz ± 3 kHz
- Complete with 6 tips
- Size: W155mm x D168mm x H80mm
- Weight: 0.6 kg (unit only)
- · Colour: White



Max Piezo 6

MaxPiezo 6+ (EMS Type) LED Scaler Set\$330.00
MaxPiezo DS6+ (SATELEC Type) LED Scaler Set\$330.00

N3000L (EMS Type) Built-In LED Scaler Set\$275.00 V3000L (SATELEC Type) Built-In LED Scaler Set\$275.00

REFINE N3000L / V3000L BUILT-IN LED SCALERS

- Automatic frequency tracking, real-time feedback
- Detachable handpiece
- Frequency: 28 KHz ± 3 KHz
- Complete with 6 tips



ONE YEAR WARRANTY (except scaler tips)

- 1. EMS is a registered trademark of Electro Medical System S.A. Switzerland
- 2. SATELEC is a registered trademark of Satelec/Acteon Group France

REFINE SCALER HANDPIECES







HS-7H Non-LED Scaler Handpiece (SATELEC² Type) \$220.00



HP-5L LED Scaler Handpiece (EMS¹ Type) \$220.00



HS-7L LED Scaler Handpiece (SATELEC² Type) \$247.50

ONE YEAR WARRANTY



REFINE SCALER TORQUE WRENCHES





TW-1L For EMS¹, KAVO PiezoLED⁵, SATELEC², NSK³ type scalers each





TS-1L For SIRONA⁴ type scalers each \$19.80

\$19.80





TK-1L For KAVO⁵, SONICflex⁵, SONOsoft⁵ type scalers each \$19.80

REFINE SCALER HANDPIECE HOSES









3H Non-LED (EMS¹ Type) Handpiece Hose ... \$59.95

7H Non-LED (SATELEC² Type) Handpiece Hose ... \$59.95









5L LED (EMS¹ Type) Handpiece Hose ... \$68.75

7L LED (SATELEC² Type) Handpiece Hose ... \$68.75

• Multi function wrench for both endo chuck & burs

- 1. EMS is a registered trademark of Electro Medical System S.A. Switzerland
- 2. SATELEC is a registered trademark of Satelec/Acteon Group France
- 3. NSK is a registered trademark of Nakanishi Inc. Japan
- 4. SIRONA is a registered trademark of Siroa Dental System
- 5. KAVO, SONICflex, SONOsoft, PiezoLED are registered trademarks of Kavo Dental GmbH Germany

REFINE SCALER TIP HOLDERS





E04 ULTRASONIC FILES NiTi alloy

- For use with ultrasonic scaler
- Excellent tenacity
- Length: 33 mm

E04 ULTRASONIC FILES NiTi alloy					
#15 🔾	#30 🔵				
#20 🛑	#35 🔵				
#25	#40 •				

E04 Ultrasonic Files Single Size 6 pcs/pack



REFINE SCALER TIPS STAINLESS STEEL

for EMS1, SATELEC2, NSK3 and SIRONA4 REFINE Type Scalers



G1 (EMS1 Type) GD1 (SATELEC², NSK³ Type) GS1 (SIRONA⁴ Type) Supragingival deposits in all quadrants

G2 (EMS¹ Type) GD2 (SATELEC², NSK³ Type) GS2 (SIRONA⁴ Type) Comparable with EMS¹ Type B Heavy supragingival deposits on anterior teeth each \$27.50

G3 Comparable with EMS¹ Type P each \$33.55

G3 (EMS1 Type) GD3 (SATELEC², NSK³ Type) GS3 (SIRONA4 Type) Supragingival deposits in all quadrants, including the interproximal and sulcus areas **SCALING**



G4 (EMS¹ Type) GD4 (SATELEC², NSK³ Type) GS4 (SIRONA⁴ Type) Supragingival and interproximal deposits



G5 (EMS¹ Type) GD5 (SATELEC², NSK³ Type) GS5 (SIRONA⁴ Type) Supragingival deposits in all quadrants



G6 (EMS¹ Type) GD6 (SATELEC², NSK³ Type) GS6 (SIRONA⁴ Type) Voluminous supragingival deposits



E1 (EMS¹ Type) ED1 (SATELEC², NSK³ Type) ES1 (SIRONA4 Type) 120°file holder for anterior root canal irrigation




E2 (EMS1 Type) ED2 (SATELEC², NSK³ Type) ES2 (SIRONA4 Type) 95°file holder for molar teeth root canal irrigation



E3 (EMS1 Type) ED3 (SATELEC2, NSK3 Type) ES3 (SIRONA4 Type) Gutta-percha melting



E3D (EMS¹ Type) ED3D (SATELEC², NSK³ Type) ES3D (SIRONA⁴ Type) Diamond coated instrument for root canal enlarging



P4D (EMS1 Type) PD4D (SATELEC², NSK³ Type) PS4D (SIRONA4 Type) Diamond coated instrument for root canal enlarging

E14 (EMS¹ Type) ED14 (SATELEC², NSK³ Type) ES14 (SIRONA⁴ Type)

Removing root filling obstructions during root canal retreatments



30.2 mn

E15

each \$49.50

E15 (EMS1 Type) ED15 (SATELEC2, NSK3 Type) ES15 (SIRONA4 Type) Removing root filling obstructions during root canal retreatments **ENDO**



E4 (EMS¹ Type) ED4 (SATELEC², NSK³ Type) ES4 (SIRONA4 Type) Removing root filling obstructions during root canal retreatment



E4D (EMS¹ Type) ED4D (SATELEC², NSK³ Type) ES4D (SIRONA⁴ Type) Removing calcification and filling material during root canal retreatment



E5 (EMS¹ Type) ED5 (SATELEC², NSK³ Type) ES5 (SIRONA4 Type) Removing root filling obstructions during root canal retreatment



ED5D (SATELEC², NSK³ Type) ES5D (SIRONA4 Type) Removing calcification and filling material during canal retreatment

E5D (EMS1 Type)



- 1. EMS is a registered trademark of Electro Medical System S.A. Switzerland
- SATELEC is a registered trademark of Satelec/Acteon Group France
 NSK is a registered trademark of Nakanishi Inc. Japan
 SIRONA is a registered trademark of Siroa Dental System

REFINE SCALER TIPS STAINLESS STEEL

for EMS1, SATELEC2, NSK3 and SIRONA4 Type Scalers



P1 (EMS1 Type) PD1 (SATELEC2, NSK3 Type) PS1 (SIRONA4 Type) Shallow pocket subgingival deposits

P3 (EMS¹ Type) PD3 (SATELEC², NSK³ Type) PS3 (SIRONA4 Type) Deep pocket subgingival deposits

P4 (EMS¹ Type) PD4 (SATELEC², NSK³ Type) PS4 (SIRONA⁴ Type) Shallow pocket subgingival deposits

P3D (EMS¹ Type) PD3D (SATELEC², NSK³ Type) PS3D (SIRONA⁴ Type) Diamond coated instrument for root planning after periodontal flap surgery

PFRIO

P2L (EMS1 Type) PD2L (SATELEC2, NSK3 Type) Left angle instrument to remove calculus from very narrow inter-root space and furcation

P2R (EMS¹ Type) PD2R (SATELEC², NSK³ Type) Right angle instrument to remove calculus from very narrow each \$38.50 inter-root space and furcation

P2LD each \$49.50 33.7 mm

P2RD

each \$49.50

P2LD (EMS¹ Type) PD2LD (SATELEC², NSK³ Type) Removal of calculus from narrow inter-root spaces (diamond-coated)

P2RD (EMS1 Type) PD2RD (SATELEC2, NSK3 Type) Diamond coated instrument for root planning

for AMDENT⁶ Type Scalers

each \$49.50



A1 (#37) (AMDENT 6 Type) Supragingival scaling



33.7 mn


A2 (#39) (AMDENT 6 Type) Supragingival scaling

Buv 2 aet **FREE** (same number)

for KAVO SONICflex⁵ Type Scalers



GK1 (KAVO5 Type) Supragingival deposits in all quadrants



GK2 (KAVO5 Type) Supragingival heavy calculus and plaque



GK3 (KAVO⁵ Type) Supragingival interdental calculus and calculus at the neck of the tooth



GK4 (KAVO5 Type) Supragingival deposits, including the interproximal and sulcus areas



GK5 (KAVO5 Type) Subgingival calculus

GK6 (KAVO5 Type)



35.8mm

Left angle instrument for reymoving subgingival calculus

GK7 (KAVO⁵ Type) Right angle instrument for revmoving subgingival

for KAVO SONOsoft⁵ Type Scalers



GC1 (KAVO5 Type) Supragingival deposits in all quadrants



GC2 (KAVO5 Type) Supragingival interdental calculus and calculus at the neck of the tooth

PC1 (KAVO⁵ Type) Subgingival calculus, including the interproximal and sulcus areas

for KAVO PiezoLED⁵ Type Scalers



201 (KAVO⁵ Type) Supragingival and interproximal deposits

202 (KAVO⁵ Type) in all quadrants, including the interproximal and sulcus areas

each \$68.75 31.4 mm

203 (KAVO⁵ Type) Deep pocket subgingival deposits

- 1. EMS is a registered trademark of Electro Medical System S.A. Switzerland
- 2. SATELEC is a registered trademark of Satelec/Acteon Group France

- 3. NSK is a registered trademark of Nakanishi Inc. Japan
 4. SIRONA is a registered trademark of Siroa Dental System
 5. KAVO, SONICflex, SONOsoft, PiezoLED are registered trademarks of Kavo Dental GmbH Germany
 6. AMDENT is a registered trademark of Amdent AB Sweeden

precisionplus*

A08 DENTAL APEX LOCATOR



- · Bright LCD screen with the trajectory of the file being clearly indicated by different colours
- Foldable design with adjustable view angle, saves space and protects the screen
- The unit is designed with a smooth seamless body and membrane buttons to enhance cold sterilization and help avoid cross contamination
- · Advanced multiple frequency technology with automatic calibrating ensures accurate measurement
- · Measurement results are not affected by tooth type, size of root canal or the internal environment of root canal
- Different beep tones indicate the position of the file in the root canal
- Rechargeable lithium battery
- Accessories autoclavable up to 134°C
- Screen size: 110 mm x 70 mm
- Overall size: L122 mm x W118 mm x H25 mm
- Weight: 300 gms (including battery)

A08-3 Spare Hook \$49.50 A08 Apex Locator \$385.00 A08-1 Battery \$59.95 A08-2 Spare Probe \$38.50 A08-4 Spare Cord \$38.50 A08-5 Spare Clip \$49.50 24 MONTH



















premium blus

C10 LED & HALOGEN CURING LIGHT METER

- · Measures intensity up to 2500 mw/cm²
- Size: 110 mm x 68 mm x 33 mm

C10 Light Meter \$59.95

24 MONTH WARRANTY



PREMIUM AP III DENTAL BURNER

- Designed for safe, one handed use
- · Battery powered ignition lights instantly with just a press of a button
- Adjustable flame setting and lock-off switch
- Burns up to 30 minutes on one butane fill-up
- Size: 14 cm long

\$396,00/set

VOODPECKER CURING IGHT ACCESSORIES

premium





Curing Light Depth Gauge each \$9.90

PREMIUM 17" LCD MONITOR



17" Monitor ... \$678.50

- Low voltage 12V
- · Reinforce glass protection for scratch resistance

- Built-in dual speakers
 On screen display control
 Auto adjustment function
- High resolution:- 1280 x 1024
- For VGA, cable TV, DVD etc
- Colour:- White

SPECIAL 395.00

MONITOR MOUNTS



- For 15" or 17" monitor
- fit 45mm post
- · Colour:- White
- Metal construction



WOODPECKER PIEZO ULTRASONIC SCALERS with endo function

UDS-E (EMS¹ TYPE) PORTABLE SCALER UDS-P (EMS¹ TYPE) TABLE TOP SCALER UDS-N3 (EMS¹ TYPE) BUILT-IN SCALER

ARE NOW AVAILABLE WITH LED LIGHT







- Digitally controlled, automatic frequency tracking
- With endo function
- · Autoclavable Titanium handpiece with excellent piezo-ceramic vibrations
- Frequency: 28kHz ± 3kHz
- DETACHABLE HANDPIECE

12 MONTH WARRANTY

(except scaler tips)

UDS-E LED Portable Scaler Set

Plastic Bottle Large 500 ml . Plastic Bottle Small 350 ml .

UDS-N3 LED (EMS1 TYPE) BUILT-IN SCALER DTE-V3 LED (SATELEC² TYPE) BUILT-IN SCALER





Size:- W8 cm x D6 cm x H4 cm

DTE-V3 LED KIT (SATELEC² TYPE)

UDS-N3 LED Kit (EMS1 Type) Built-in LED Scaler with 6 Tips (G1T x 2, G2T, G4T, P1T and E1T) DTE-V3 LED Kit (SATELEC² Type) Built-in LED Scaler with 6 Tips (GD1T x 2, GD2T, GD4T, PD1T and ED1T)\$396.00

> 1. EMS is a registered trademark of Electro Medical System S.A. Switzerland 2. SATELEC is a registered trademark of Satelec/Acteon Group France



OODPECKER TITANIUM SCALER HANDPIECES



HW-3H (Woodpecker, EMS¹ Type) Non-LED Scaler Handpiece .. \$247.50







HD-7H (DTE, SATELEC² Type) Non-LED Scaler Handpiece .. \$275.00









HW-5L (Woodpecker, EMS¹ Type) LED Scaler Handpiece \$275.00

HD-7L (DTE, SATELEC² Type) LED Scaler Handpiece \$291.50

12 MONTH WARRANTY



1. EMS is a registered trademark of Electro Medical System S.A. Switzerland 2. SATELEC is a registered trademark of Satelec/Acteon Group France

WOODPECKER SCALER TIPS STAINLESS STEEL

for WOODPECKER, EMS1, DTE, SATELEC2, NSK3 or SIRONA4 Type Scalers



CAVITY PREPARATION



₹SB1

SB1 (WOODPECKER, EMS1 Type) SBD1 (DTE, SATELEC2, NSK3 Type) For occlusal surface and cervical margins preparation



SB3 (WOODPECKER, EMS1 Type) SBD3 (DTE, SATELEC2, NSK3 Type) Remove the carious teeth without damaging the adjacent teeth



SBL (WOODPECKER, EMS1 Type) SBDL (DTE, SATELEC2, NSK3 Type) Half ball diamond tip. Set 45° to the left, to remove the carious teeth without damaging the adjacent teeth.




SBR (WOODPECKER, EMS1 Type) SBDR (DTE, SATELEC2, NSK3 Type) Half ball diamond tip. Set 45° to the right, to remove the carious teeth without damaging the adjacent teeth.

- 1. EMS is a registered trademark of Electro Medical System S.A. Switzerland
- 2. SATELEC is a registered trademark of Satelec/Acteon Group France 3. NSK is a registered trademark of Nakanishi Inc. Japan
- 4. SIRONA is a registered trademark of Siroa Dental System

WOODPECKER SCALER TIPS STAINLESS STEEL for WOODPECKER, EMS1, DTE, SATELEC2, NSK3 or SIRONA3 Type Scalers



WOODPECKER SCALER TIPS STAINLESS STEEL for AMDENT® Type Scaler

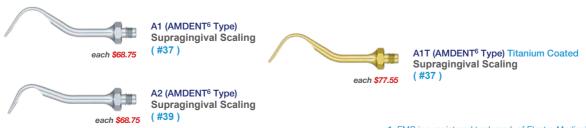

- 1 EMS is a registered trademark of Electro Medical System S.A. Switzerland
 2 SATELEC is a registered trademark of Satelec/Acteon Group France
 3 NSK is a registered trademark of Nakanishi Inc. Japan

- 4 SIRONA is a registered trademark of Siroa Dental System 6 AMDENT is a registered trademark of Amdent AB Sweeden

WOODPECKER SCALER TIPS STAINLESS STEEL TITANIUM COATED Non-Sticky, Longer Lasting for WOODPECKER, EMS¹, DTE, SATELEC², NSK³ Type Scalers





- Working time:- 10 seconds
- Three work modes:- Full, Ramping, Pulse
- Autoclavable Light Guide 8mm
- Light weight:- 90-135gms
- Attractive slim design
- Sizes:- L250mm x Dia. 31-34mm
- Complete with protective light shield and composite curing depth gauge

WOODPECKER SCALER TIPS STAINLESS STEEL for KAVO⁵ Type Scalers



GK1 (KAVO⁵ Type) SONICflex⁵ Type Supragingival and Subgingival Scaling



GK2 (KAVO⁵ Type) SONICflex⁵ Type Supragingival and Subgingival Scaling



GK3 (KAVO5 Type) SONICflex⁵ Type Supragingival and Subgingival Scaling



GK4 (KAVO⁵ Type) SONICflex⁵ Type Supragingival and Subgingival Scaling



GK5 (KAVO5 Type) SONICflex⁵ Type Supragingival and Subgingival Scaling



GK6 (KAVO⁵ Type) SONICflex⁵ Type Supragingival and Subgingival Scaling



GK7 (KAVO5 Type) SONICflex⁵ Type Supragingival and Subgingival Scaling



EK8 (KAVO5 Type) SONICflex⁵ Type Bur Holder, to enlarge root canal



GC1 (KAVO⁵ Type) SONOsoft⁵ Type Supragingival and Subgingival Scaling



GC2 (KAVO5 Type) SONOsoft⁵ Type Supragingival and Subgingival Scaling



PC1 (KAVO⁵ Type) SONOsoft⁵ Type Subgingival Scaling

- 1 EMS is a registered trademark of Electro Medical System S.A. Switzerland
- 2 SATELEC is a registered trademark of Satelec/Acteon Group France 3 NSK is a registered trademark of Nakanishi Inc. Japan
- S A SIRONA is a registered trademark of Siroa Dental System
 KAVO, SONICflex, SONOsoft are registered trademarks of Kavo Dental GmbH Germany



WOODPECKER **TOROUE WRENCHES**

- Autoclavable
- · Holds Scaler tip inside
- · Colour: White

TW-1L Torque Wrench (WOODPECKER, EMS¹ Type) \$27.50 TD-1L Torque Wrench (DTE, SATELEC², NSK³ Type) \$27.50 TS-1L Torque Wrench (SIRONA⁴ Type) \$27.50



WOODPECKER SCALER ACCESSORIES











WOODPECKER SCALER HANDPIECE CABLES

Scaler Handpiece Cable (WOODPECKER, EMS¹ Type)... \$68.75 Scaler Handpiece Cable (DTE, SATELEC² Type).........................\$68.75 LED Scaler Handpiece Cable (WOODPECKER, EMS' Type) ... \$79.75 LED Scaler Handpiece Cable (DTE, SATELEC' Type) \$79.75



WOODPECKER SCALER U-FILES

- Excellent tenacity
- 6 pieces per tube
- Length: 32.5 mm

U-Files, 6 pcs/tube No.20, 30, 35 \$16.50



REFINE SCALER HANDPIECES





HP-3H Non-LED Scaler Handpiece (EMS1 Type) \$198.00







HP-5L LED Scaler Handpiece (EMS1 Type) \$220.00

HS-7L LED Scaler Handpiece (SATELEC2 Type) \$247.50

ONE YEAR WARRANTY

- Buy 2 aet
- 1. EMS is a registered trademark of Electro Medical System S.A. Switzerland
- 2. SATELEC is a registered trademark of Satelec/Acteon Group France

REFINE AUTOCLAVABLE SCALER HANDPIECE KITS

- · Complete with:-1x Handpiece 3H / 5L / 7H / 7L
- 3x Perio scaler tip P1 / PD1
- 1x Torque wench TW-1L
- 1x Scaler tip holder No.1
- 1x Sterilization box



3H Non-LED Handpiece Kit (EMS Type) 7H Non-LED Handpiece Kit (SATELEC Type) \$330.00 5L LED Handpiece Kit (EMS Type) 7L LED Handpiece Kit (SATELEC Type)\$38 (for handpiece connections, please refer to above)

SPECIAL 3H Kit \$198.00 7H Kit \$220.00 5L (LED) Kit \$220.00 7L (LED) Kit \$247.50



REFINE MaxPiezo 7+ / DS7+ PORTABLE LED SCALERS

- Automatic frequency tracking, real-time feedback
- Extra large, capacity 600 ml water tank for water, chlorhexidine, hydrogen peroxide, sodium hypochlorite etc...
- Power and water controlled by touch panel, easy to clean for infection control
- Detachable handpiece
- Frequency: 28 kHz ± 3 kHz
- Complete with 8 tips as shown
- Size: W180mm x D180mm x H150mm
- Weight: 1.6 kg (unit only)
- · Colour: White

MaxPiezo 7+ (EMS Type) Portable LED Scaler Set\$880.00
MaxPiezo DS7+ (SATELEC Type) Portable LED Scaler Set ... \$880.00



REFINE MaxPiezo 6+ / DS6+ LED SCALERS



- Automatic frequency tracking, real-time feedback
- · Power and water controlled by touch panel, easy to clean for infection control
- Detachable handpiece
- Frequency: 28 kHz ± 3 kHz
- · Complete with 6 tips as shown
- Size: W155mm x D168mm x H80mm
- Weight: 0.6 kg (unit only)
- · Colour: White

MaxPiezo 6+ (EMS Type) LED Scaler Set .. MaxPiezo DS6+ (SATELEC Type) LED Scaler Set \$330.00



ONE YEAR WARRANTY (except scaler tips)



1. EMS is a registered trademark of Electro Medical System S.A. Switzerland 2. SATELEC is a registered trademark of Satelec/Acteon Group France